


Chart Note

Current Medical Technologies, Inc.

Patient Name: Jane Doe
Patient DOB: 07/16/1966
Date of Visit: 1/5/2017 3:15:24PM
Provider: Earl Carlow


Care Administered by: **Earl Carlow**

• **Electro Myography (EMG):**

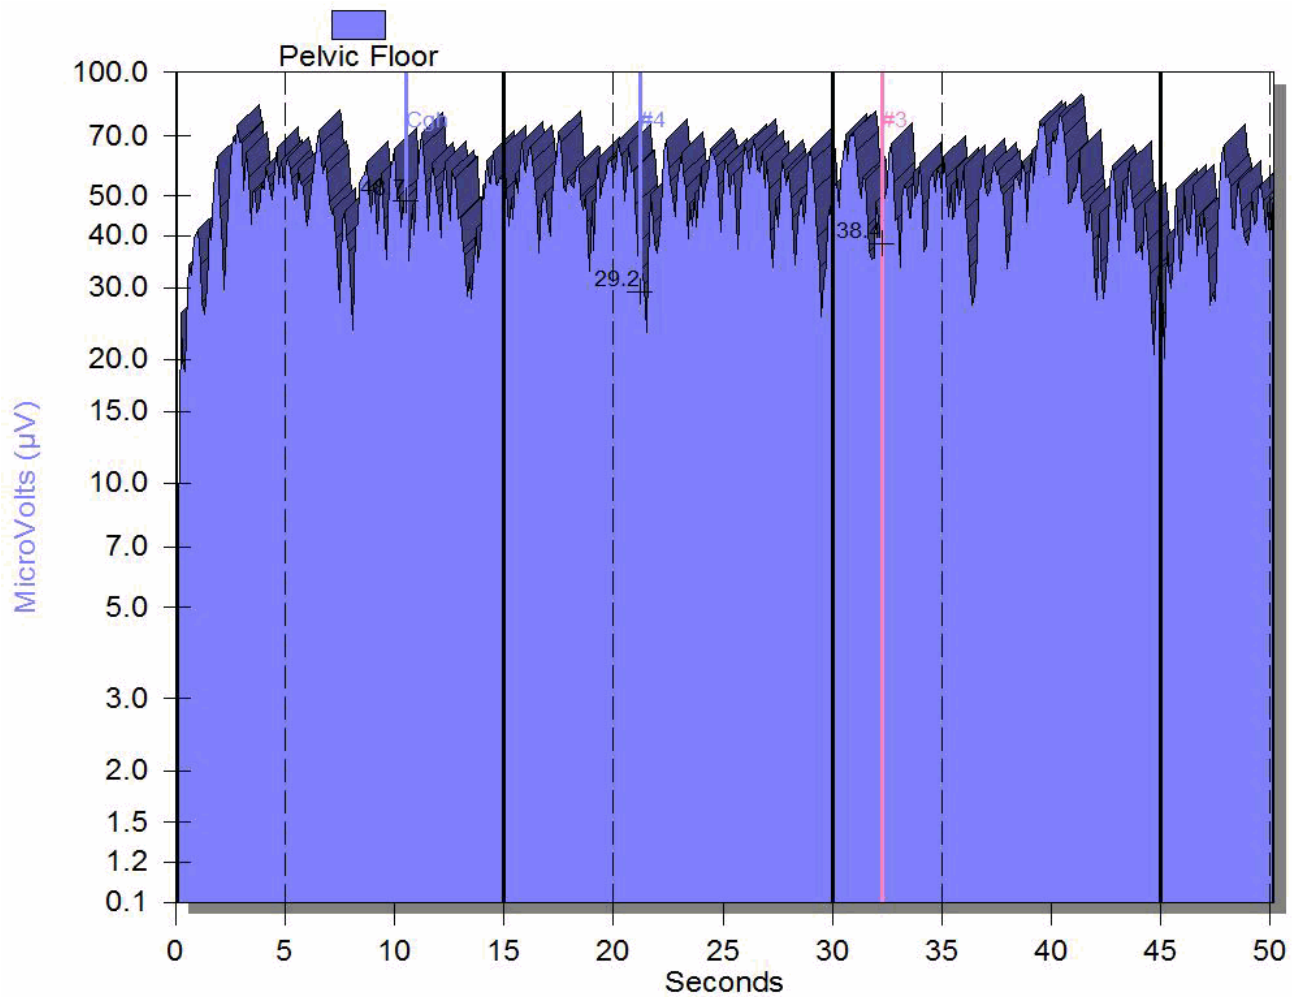

Patient Name:

Jane Doe

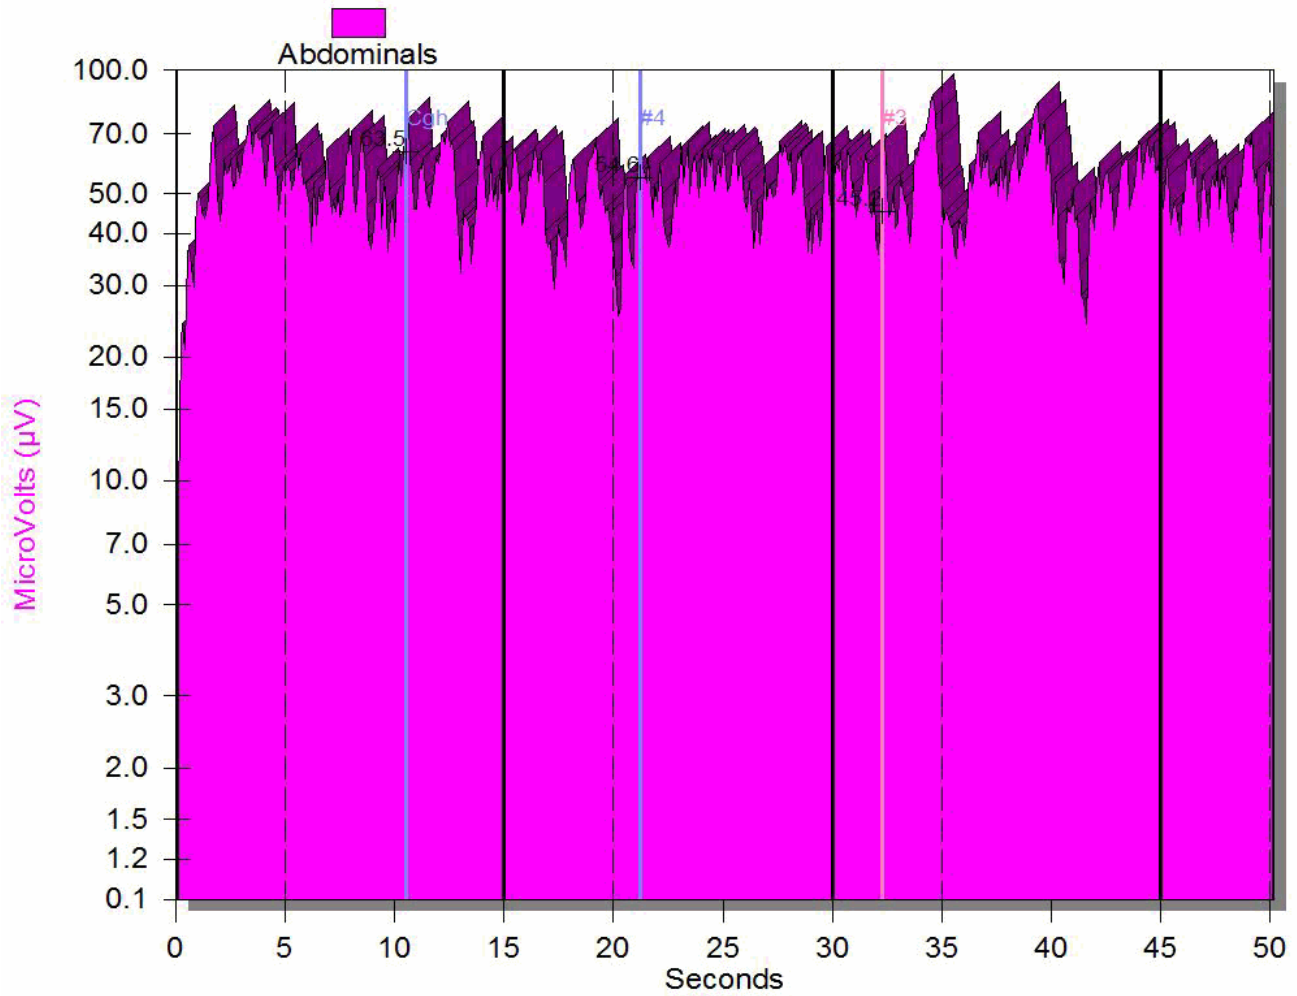

Overall Treatment Values:

EMG A	Avg(µV)	Min(µV)	Max(µV)	W-R Rise(µV)
Work	49.1	20.1	74.5	-1.36
Rest	50.5	20.6	78.6	
EMG B	Avg(µV)	Min(µV)	Max(µV)	W-R Rise(µV)
Work	53.0	29.4	87.4	-0.28
Rest	53.2	24.2	83.8	

Individual Trial Values:


EMG A	Avg(µV)	Min(µV)	Max(µV)	W-R Rise(µV)
Work 1	48.2	42.8	74.5	-1.06
Rest 1	49.2	23.6	72.4	
Work 2	53.2	33.0	71.6	2.31
Rest 2	50.9	23.4	68.6	
Work 3	51.9	33.6	71.6	2.16
Rest 3	49.8	20.6	78.6	
Work 4	43.1	20.1	66.7	-5.02
Rest 4	48.1	48.1	48.1	

Patient Name: Jane Doe


EMG B	Avg(μ V)	Min(μ V)	Max(μ V)	W-R Rise(μ V)
Work 1	53.5	45.6	75.4	0.29
Rest 1	53.2	32.3	76.3	
Work 2	50.1	29.4	67.9	-1.77
Rest 2	51.8	25.3	67.2	
Work 3	55.9	35.6	87.4	2.66
Rest 3	53.2	24.2	83.8	
Work 4	52.5	36.2	70.7	8.11
Rest 4	44.3	44.3	44.3	

Custom Marker	Latency (mm:ss.t)	EMGA (μ V)	EMGB (μ V)	
Cough	00:10.5	37.31	72.35	0.00
Marker 4	00:21.2	29.18	54.59	0.00
Marker 3	00:32.3	49.53	57.66	0.00

• Electro Myography (EMG):

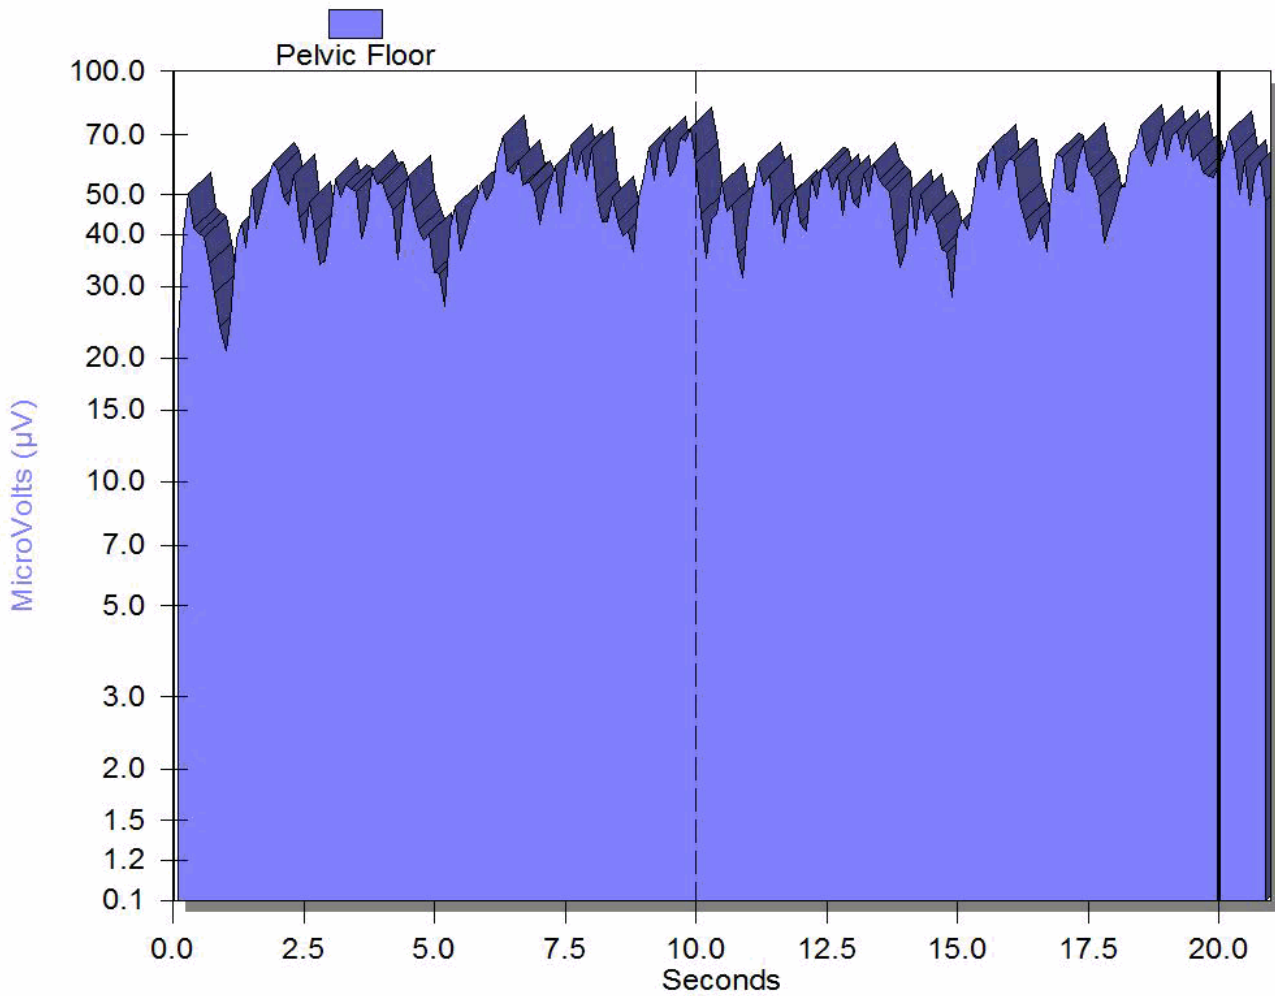

Patient Name: Jane Doe

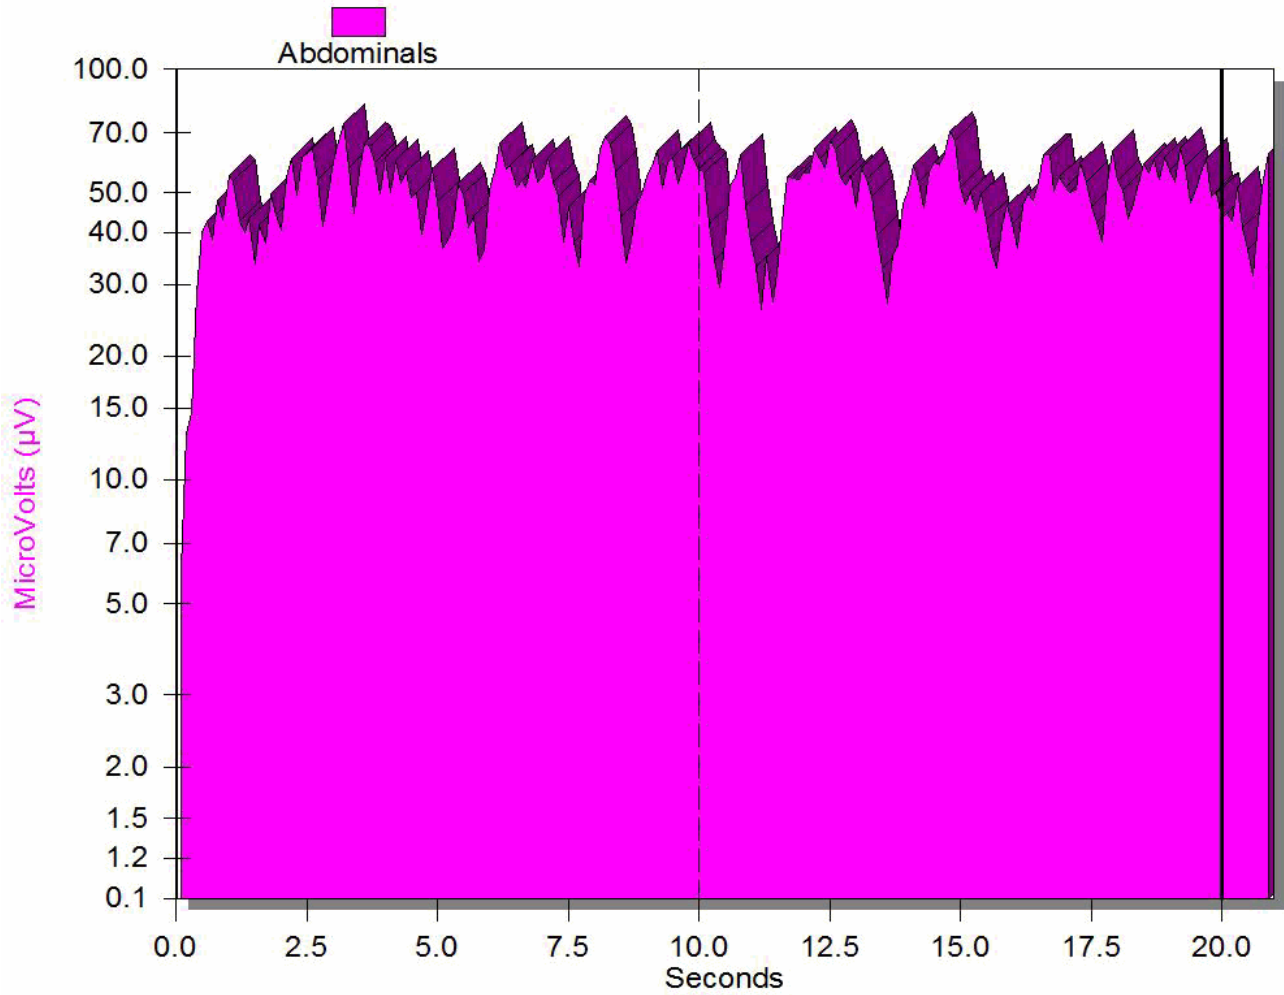

Overall Treatment Values:

EMG A	Avg(µV)	Min(µV)	Max(µV)	W-R Rise(µV)
Work	49.0	26.8	72.9	-2.24
Rest	51.3	28.1	74.0	

EMG B	Avg(µV)	Min(µV)	Max(µV)	W-R Rise(µV)
Work	50.0	31.5	73.6	0.07
Rest	49.9	25.9	70.4	


Individual Trial Values:

EMG A	Avg(µV)	Min(µV)	Max(µV)	W-R Rise(µV)
Work 1	48.3	26.8	72.9	-3.02
Rest 1	51.3	28.1	74.0	
Work 2	57.8	47.2	70.9	57.76
Rest 2	0.0	0.0	0.0	


EMG B	Avg(µV)	Min(µV)	Max(µV)	W-R Rise(µV)
Work 1	50.4	33.1	73.6	0.50
Rest 1	49.9	25.9	70.4	
Work 2	45.3	31.5	62.3	45.30
Rest 2	0.0	0.0	0.0	

Patient Name: Jane Doe

• Electro Myography (EMG):

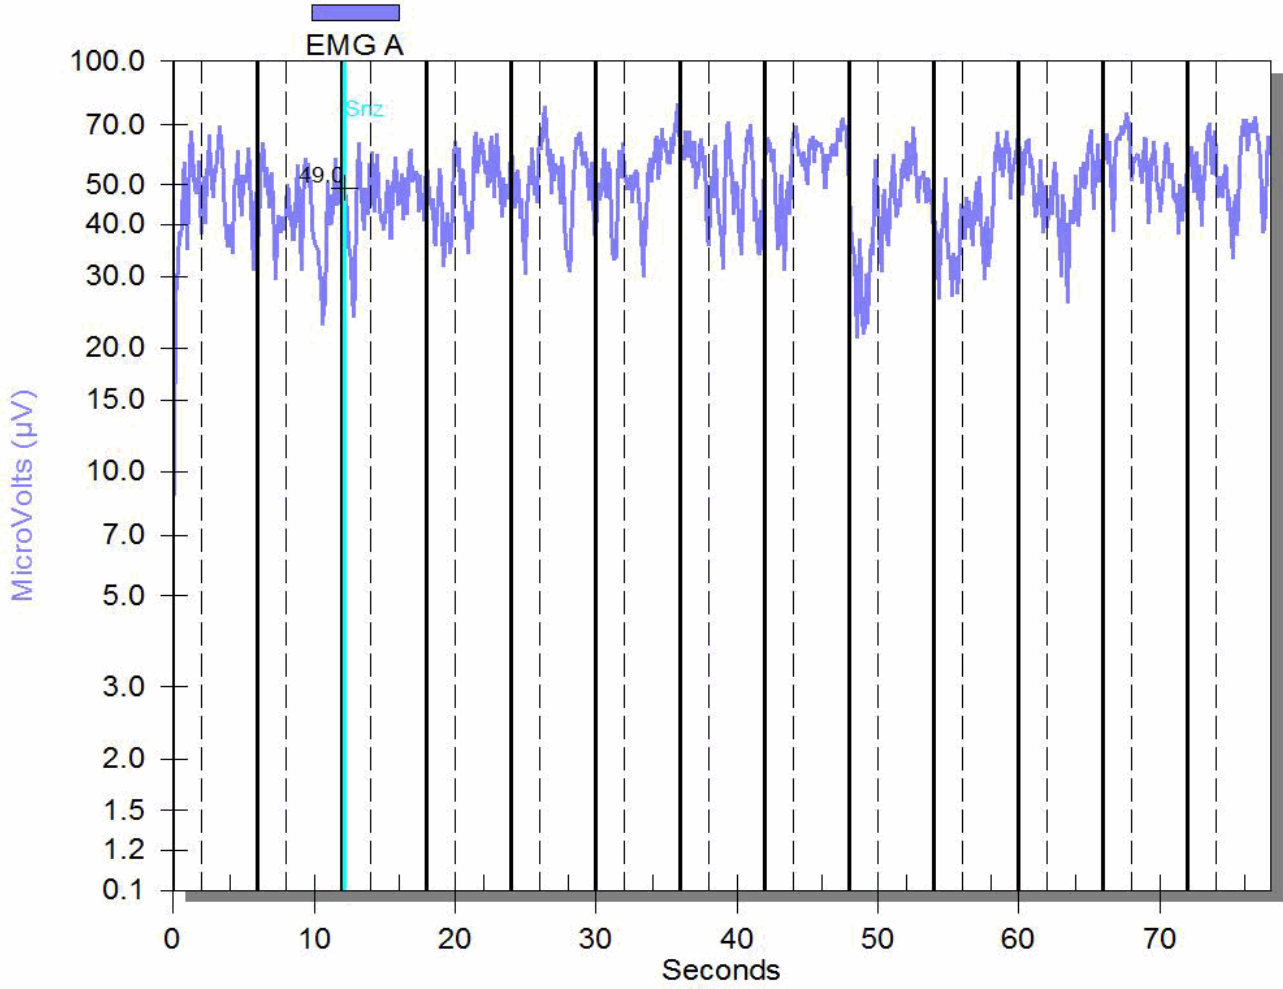

Patient Name: Jane Doe

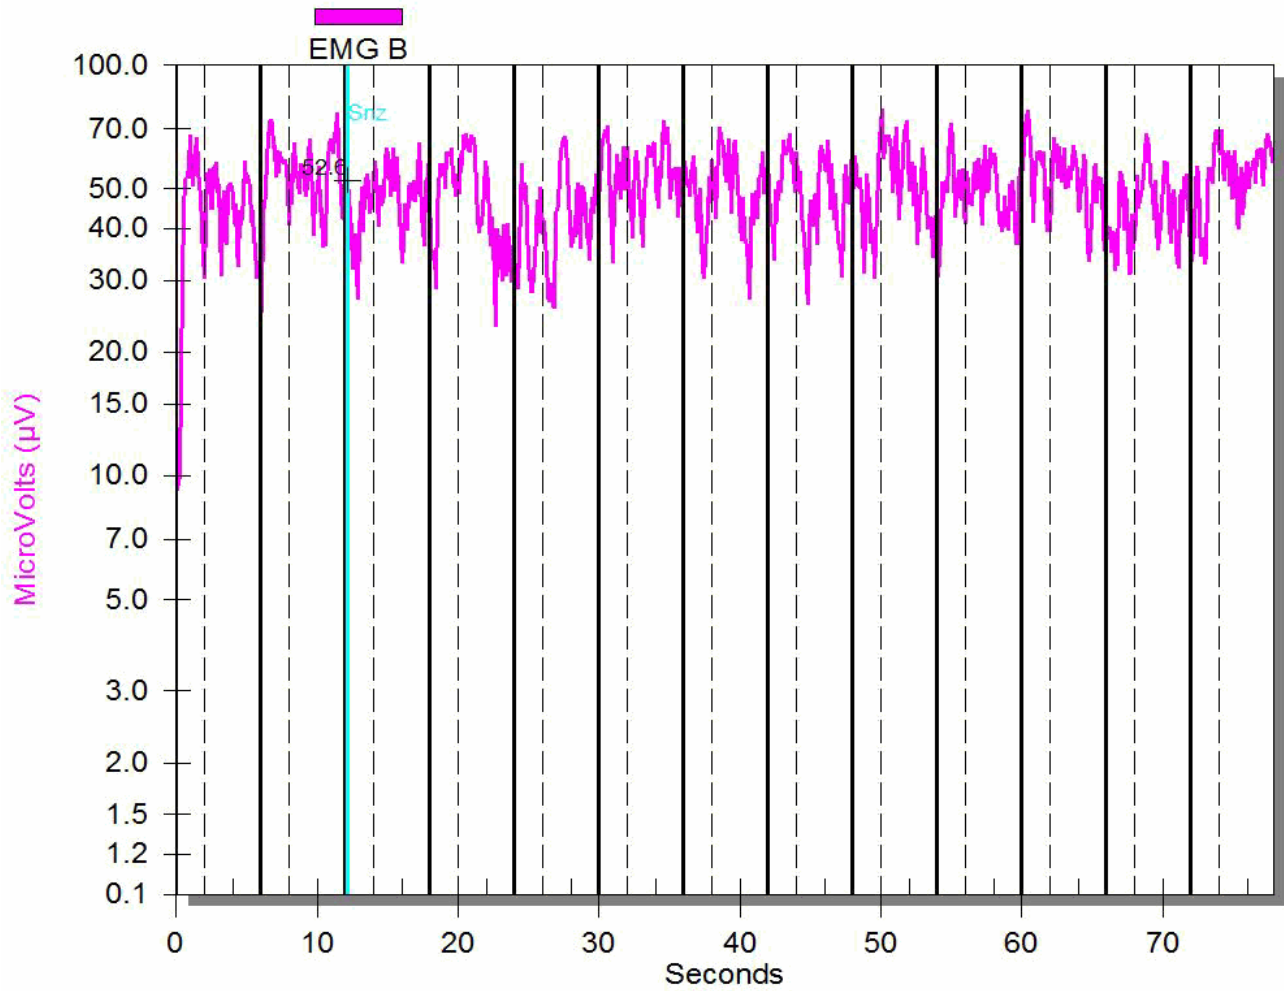

Overall Treatment Values:

EMG A	Avg(µV)	Min(µV)	Max(µV)	W-R Rise(µV)
Work	48.1	21.1	75.0	-4.35
Rest	52.4	22.8	78.8	
EMG B	Avg(µV)	Min(µV)	Max(µV)	W-R Rise(µV)
Work	49.2	25.1	77.7	-2.05
Rest	51.2	23.2	78.5	

Current Medical Technologies, Inc.

Patient Name: Jane Doe

Individual Trial Values:

EMG A	Avg(µV)	Min(µV)	Max(µV)	W-R Rise(µV)
Work 1	47.1	1,000.0	67.7	-2.17
Rest 1	49.3	30.9	69.8	
Work 2	45.4	29.4	63.2	2.72
Rest 2	42.7	22.8	58.2	
Work 3	42.7	23.8	63.4	-5.78
Rest 3	48.5	37.0	61.1	
Work 4	44.1	31.7	63.6	-8.82
Rest 4	52.9	34.0	67.3	
Work 5	48.6	30.2	65.6	-5.18
Rest 5	53.7	30.8	77.5	
Work 6	49.2	32.9	63.4	-6.19
Rest 6	55.4	29.9	78.8	
Work 7	56.2	35.6	67.7	6.77
Rest 7	49.4	31.3	71.1	
Work 8	50.7	31.1	67.0	-10.31
Rest 8	61.0	48.7	72.7	
Work 9	34.1	21.1	57.6	-15.01
Rest 9	49.1	30.9	68.9	
Work 10	36.5	26.5	52.1	-12.36
Rest 10	48.8	29.5	67.4	
Work 11	52.1	38.3	64.8	4.35
Rest 11	47.7	25.8	68.0	
Work 12	61.3	38.4	75.0	8.68
Rest 12	52.6	37.9	65.1	
Work 13	56.7	39.8	70.9	2.36
Rest 13	54.4	33.0	73.2	

EMG B	Avg(µV)	Min(µV)	Max(µV)	W-R Rise(µV)
Work 1	45.4	1,000.0	67.6	0.95
Rest 1	44.5	30.4	58.3	
Work 2	57.1	25.1	73.6	3.24
Rest 2	53.9	36.2	76.4	
Work 3	44.0	26.9	65.7	-5.89
Rest 3	49.9	33.1	65.0	
Work 4	50.6	28.6	63.0	4.30
Rest 4	46.3	23.2	68.3	
Work 5	39.9	27.9	57.4	-4.84
Rest 5	44.7	25.6	66.9	
Work 6	55.3	33.0	71.3	1.26
Rest 6	54.1	36.0	73.2	
Work 7	47.4	30.4	60.0	-3.50
Rest 7	50.9	26.9	70.8	
Work 8	53.5	33.6	67.9	6.43
Rest 8	47.1	26.3	65.5	
Work 9	48.1	30.3	72.3	-5.25
Rest 9	53.4	34.0	78.5	
Work 10	51.2	30.6	71.9	1.51
Rest 10	49.7	36.5	63.9	
Work 11	56.7	39.5	77.7	5.07
Rest 11	51.7	33.4	66.6	
Work 12	40.8	31.0	55.2	-7.69
Rest 12	48.5	32.1	68.2	
Work 13	49.4	33.0	69.4	-7.14
Rest 13	56.6	40.0	69.9	

Patient Name: Jane Doe

Custom Marker	Latency (mm:ss.t)	EMGA (μV)	EMGB (μV)	
Sneeze	00:12.2	48.95	52.56	0.00